



Laboratory Investigation Report


BML266341

Name : Ms. SHAYNA LORAIN PAJAS MUNIZ
DOB : 04/12/1991
Age / Gender : 31 Y 9 M / Female
Referred by : Dr. Enomen Goodluck Ekata
Centre : Peshawar Medical Center LLC

Ref No. : 38497
Sample No. : 2309269759
Collected : 15/09/2023 11:00
Registered : 15/09/2023 16:55
Reported : 15/09/2023 22:43

BIOCHEMISTRY

Test	Result	Flag	Unit	Reference Range	Methodology
AMYLASE TOTAL	55		U/L	25 - 115	CNP-triose/CNPG3 U/L @ 37°
LIPASE	80		U/L	73 - 393 * (*Siemens kit insert)	Colorimetric

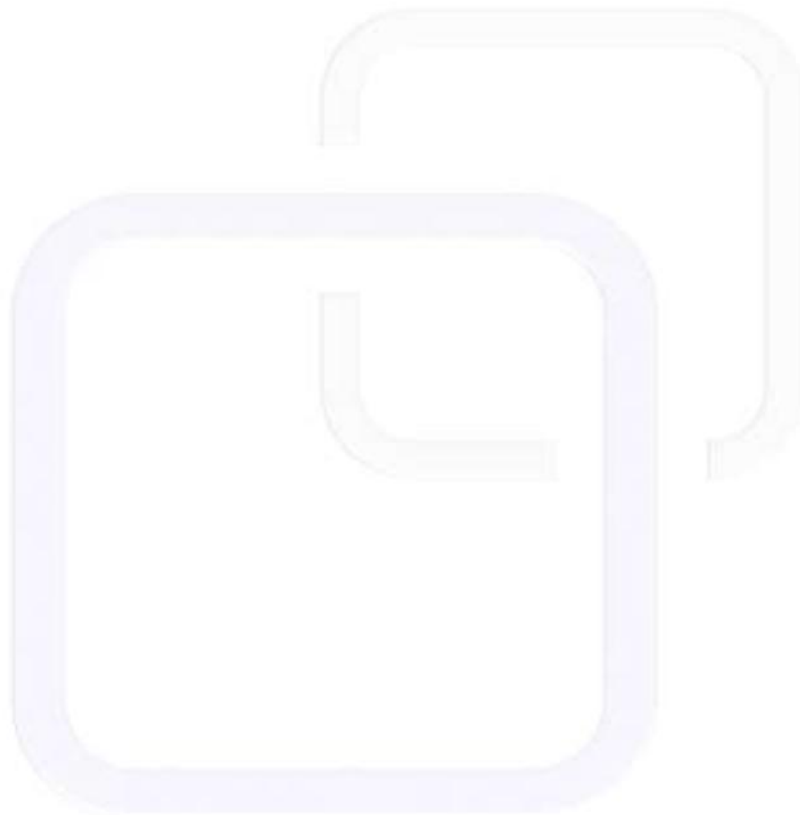

Dr. Adley Mark Fernandes

M.D (Pathology)

Pathologist

This is an electronically authenticated report

Page 1 of 2

HARSHAD MANIKANDAN

Laboratory Technician

Printed on: 16/09/2023 19:35

Test result pertains only to the sample tested and to be interpreted in the light of clinical history. These tests are accredited under ISO 15189:2012 unless specified by (^). Test marked with # is performed in an accredited referral laboratory.





Laboratory Investigation Report

BML266341

Name : Ms. SHAYNA LORAIN PAJAS MUNIZ
DOB : 04/12/1991
Age / Gender : 31 Y 9 M / Female
Referred by : Dr. Enomen Goodluck Ekata
Centre : Peshawar Medical Center LLC


Ref No. : 38497
Sample No. : 2309269759
Collected : 15/09/2023 11:00
Registered : 15/09/2023 16:55
Reported : 15/09/2023 23:20

SEROLOGY

Test	Result	Flag	Unit	Reference Range	Methodology
HELICOBACTER PYLORI ANTIBODY	Negative			Negative	Immunochromatography

Sample Type : Serum

End of Report

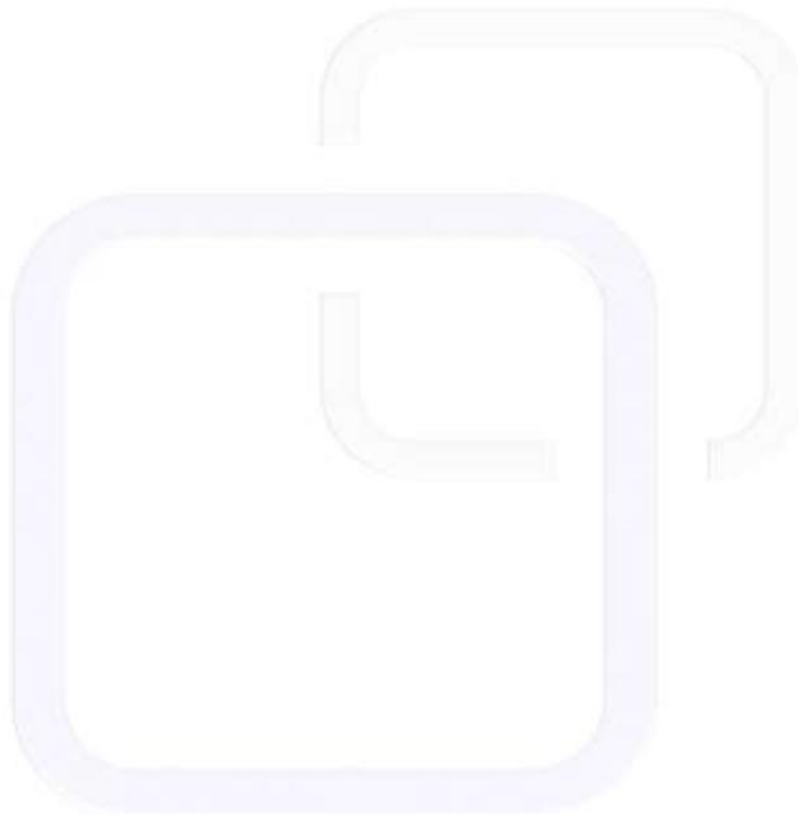

Dr. Adley Mark Fernandes

M.D (Pathology)

Pathologist

This is an electronically authenticated report

Page 2 of 2

NAZAR MOHAMED ALI

Laboratory Technologist

Printed on: 16/09/2023 19:35

Test result pertains only to the sample tested and to be interpreted in the light of clinical history. These tests are accredited under ISO 15189:2012 unless specified by (^). Test marked with # is performed in an accredited referral laboratory.

