


Laboratory Investigation Report



BML279525


Name	: Ms. EBAR A Y AL MUSA	Ref No.	: 35749
DOB	: 06/10/1971	Sample No.	: 2310283032
Age / Gender	: 52 Y / Female	Collected	: 06/10/2023 11:00
Referred by	: DR. MAHDI	Registered	: 06/10/2023 18:19
Centre	: Peshawar Medical Center LLC	Reported	: 06/10/2023 20:08

BIOCHEMISTRY

Test	Result	Flag	Unit	Reference Range	Methodology
C-REACTIVE PROTEIN (CRP)	15.1	CH	mg/L	< 5.0 Please note change in reference range.	Immunoturbidimetry

Sample Type : Serum

End of Report

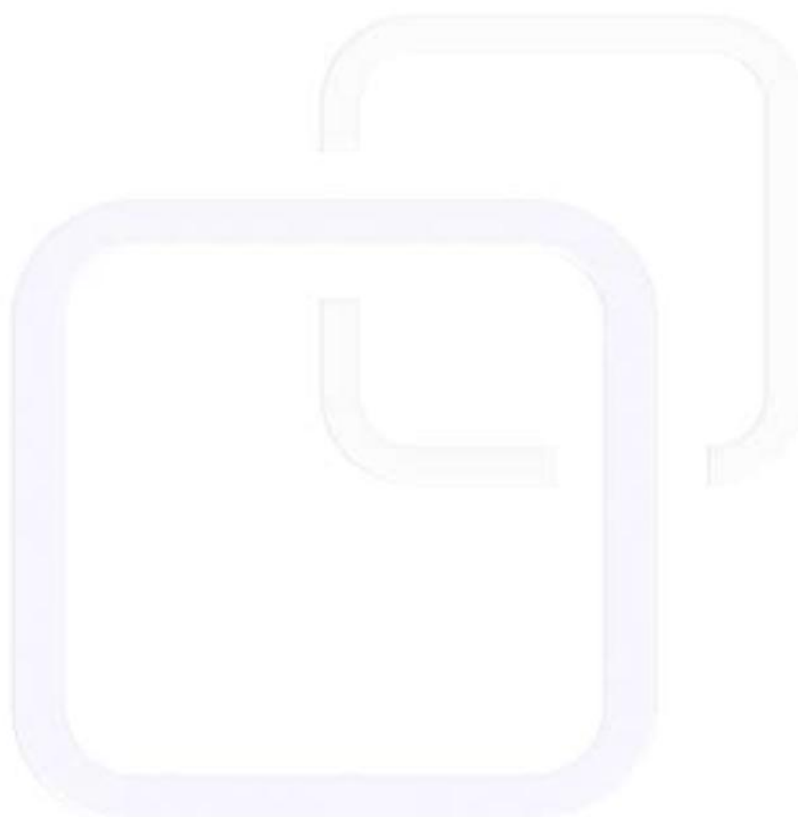

Dr. Adley Mark Fernandes
M.D (Pathology)
Pathologist

Dr. Vyoma V Shah
M.D (Pathology)
Clinical Pathologist

This is an electronically authenticated report


Page 1 of 3


SAGAR MURUKESAN PILLAI MOLY
Laboratory Technologist
Printed on: 06/10/2023 22:27

Test result pertains only to the sample tested and to be interpreted in the light of clinical history. These tests are accredited under ISO 15189:2012 unless specified by (^). Test marked with # is performed in an accredited referral laboratory.



Laboratory Investigation Report



BML279525

Name : Ms. EBAR A Y AL MUSA
DOB : 06/10/1971
Age / Gender : 52 Y / Female
Referred by : DR. MAHDI
Centre : Peshawar Medical Center LLC

Ref No. : 35749
Sample No. : 2310283032
Collected : 06/10/2023 11:00
Registered : 06/10/2023 18:19
Reported : 06/10/2023 22:25

HEMATOLOGY

Test	Result	Flag	Unit	Reference Range	Methodology
COMPLETE BLOOD COUNT (CBC)					
HEMOGLOBIN	11.8	L	g/dL	12 - 15.5	Spectrophotometry (Oxyhemoglobin)
RBC COUNT	4.5		10 ⁶ /μL	3.9 - 5	Electrical Impedance
HEMATOCRIT	35.5		%	35 - 45	Calculation
MCV	79	L	fL	82 - 98	Calculation
MCH	26.3	L	pg	27 - 32	Calculation
MCHC	33.3		g/dL	32 - 37	Calculation
RDW	20.1	H	%	11.9 - 15.5	Calculation
RDW-SD	54.7		fL		Calculation
MPV	9		fL	7.6 - 10.8	Calculation
PLATELET COUNT	267		10 ³ /μL	150 - 450	Electrical Impedance
PCT	0.2		%	0.01 - 9.99	Calculation
PDW	16.7		Not Applicable	0.1 - 99.9	Calculation
NUCLEATED RBC (NRBC) [^]	0		/100 WBC		Flow Cytometry
ABSOLUTE NRBC COUNT [^]	0		10 ³ /uL		Calculation
EARLY GRANULOCYTE COUNT (EGC) [^]	0.9		%		Flow Cytometry
ABSOLUTE EGC [^]	0.1		10 ³ /uL		Calculation
WBC COUNT	5.6		10 ³ /μL	4 - 11	Electrical Impedance
DIFFERENTIAL COUNT (DC)					
NEUTROPHILS	73		%	40 - 75	Flow Cytometry
LYMPHOCYTES	19	L	%	30 - 60	Flow Cytometry
EOSINOPHILS	2		%	0 - 6	Flow Cytometry
MONOCYTES	6		%	1 - 6	Flow Cytometry
BASOPHILS	0		%	0 - 1	Flow Cytometry
ABSOLUTE COUNT					
ABSOLUTE NEUTROPHIL COUNT	4		10 ³ /uL	1.6 - 8.25	Calculation
ABSOLUTE LYMPHOCYTE COUNT	0.9	L	10 ³ /uL	1.2 - 6.6	Calculation
ABSOLUTE MONOCYTE COUNT	0.5		10 ³ /uL	0.04 - 0.66	Calculation
ABSOLUTE EOSINOPHIL COUNT	0.1		10 ³ /uL	0 - 0.66	Calculation
ABSOLUTE BASOPHIL COUNT	0		10 ³ /uL	0 - 0.11	Calculation

Dr. Adley Mark Fernandes
M.D (Pathology)
Pathologist

Dr. Vyoma V Shah
M.D (Pathology)
Clinical Pathologist



MIDHUN MANIKANDAN GEETHA
Laboratory Technologist

This is an electronically authenticated report


Page 2 of 3

Printed on: 06/10/2023 22:27

Test result pertains only to the sample tested and to be interpreted in the light of clinical history. These tests are accredited under ISO 15189:2012 unless specified by (^). Test marked with # is performed in an accredited referral laboratory.



Laboratory Investigation Report



BML279525

Name : Ms. EBAR A Y AL MUSA
DOB : 06/10/1971
Age / Gender : 52 Y / Female
Referred by : DR. MAHDI
Centre : Peshawar Medical Center LLC

Ref No. : 35749
Sample No. : 2310283032
Collected : 06/10/2023 11:00
Registered : 06/10/2023 18:19
Reported : 06/10/2023 22:25

HEMATOLOGY


Test	Result	Flag	Unit	Reference Range	Methodology
------	--------	------	------	-----------------	-------------

COMPLETE BLOOD COUNT (CBC)

Interpretation Notes : Please note update on CBC report format and changes in reference ranges.

Sample Type : EDTA Whole Blood

End of Report

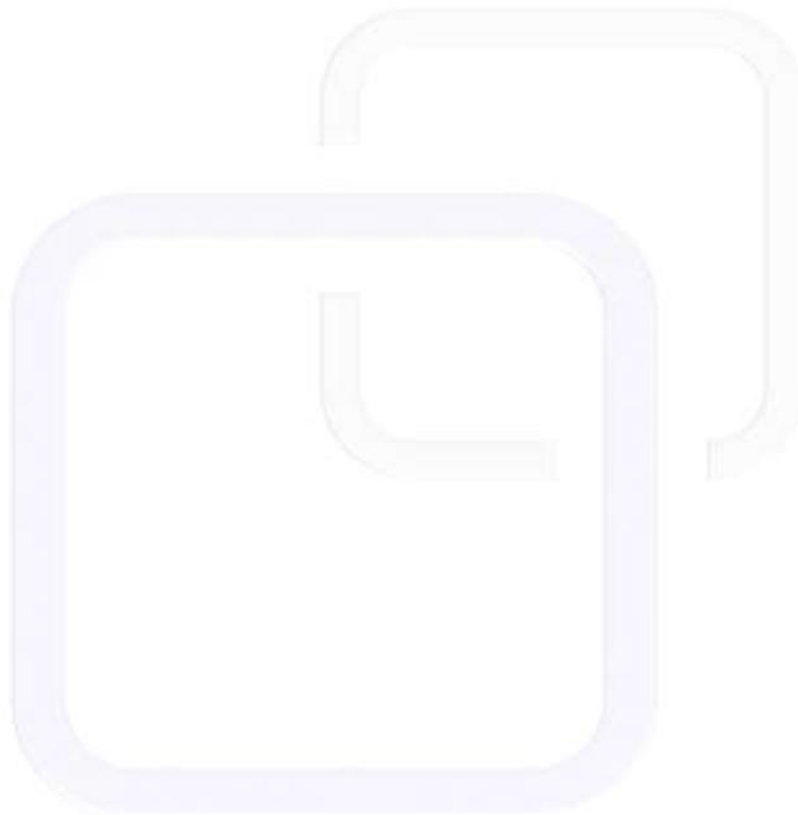

Dr. Adley Mark Fernandes
M.D (Pathology)
Pathologist

Dr. Vyoma V Shah
M.D (Pathology)
Clinical Pathologist

This is an electronically authenticated report

Page 3 of 3

MIDHUN MANIKANDAN GEETHA
Laboratory Technologist

Printed on: 06/10/2023 22:27

Test result pertains only to the sample tested and to be interpreted in the light of clinical history. These tests are accredited under ISO 15189:2012 unless specified by (^). Test marked with # is performed in an accredited referral laboratory.

