

Laboratory Investigation Report

BML282607

Name	: Ms. JOHARI DONDAPATI	Ref No.	: 41133
DOB	: 26/04/1973	Sample No.	: 2310286160
Age / Gender	: 50 Y / Female	Collected	: 11/10/2023 11:00
Referred by	: DR RASHMI	Registered	: 11/10/2023 13:38
Centre	: Peshawar Medical Center LLC	Reported	: 11/10/2023 15:25

BIOCHEMISTRY

Test	Result	Flag	Unit	Reference Range	Methodology
URIC ACID (SERUM)	4.0		mg/dL	2.6 - 6.0	Uricase, UV
CREATININE (SERUM)	0.62		mg/dL	0.59 - 1.04	Alkaline picrate (IFCC standardised)

Interpretation Notes :

Please note update in reference range with effect from 31/10/2020 (Source: Mayo Clinical Laboratories).

UREA (SERUM)	18		mg/dL	14.98 - 38.52	Kinetic test with urease and glutamate
--------------	----	--	-------	---------------	--

Dr. Adley Mark Fernandes
M.D (Pathology)
Pathologist

Dr. Vyoma V Shah
M.D (Pathology)
Clinical Pathologist

This is an electronically authenticated report

Page 1 of 4


BHAVYA THENDANKANDY
Biochemistry Technologist
Printed on: 11/10/2023 16:13

Test result pertains only to the sample tested and to be interpreted in the light of clinical history. These tests are accredited under ISO 15189:2012 unless specified by (^). Test marked with # is performed in an accredited referral laboratory.



Laboratory Investigation Report



BML282607

Name	: Ms. JOHARI DONDAPATI	Ref No.	: 41133
DOB	: 26/04/1973	Sample No.	: 2310286160
Age / Gender	: 50 Y / Female	Collected	: 11/10/2023 11:00
Referred by	: DR RASHMI	Registered	: 11/10/2023 13:38
Centre	: Peshawar Medical Center LLC	Reported	: 11/10/2023 15:25

BIOCHEMISTRY

Test	Result	Flag	Unit	Reference Range	Methodology
LIPID PROFILE TEST					
CHOLESTEROL (TOTAL)	230	H	mg/dl	Desirable: < 200 Borderline High: 200 - 240 High: > 240	Enzymatic colorimetric assay
HDL CHOLESTEROL	65	H	mg/dl	40 - 60	Homogeneous enzymatic colorimetric assay
LDL CHOLESTEROL DIRECT	142	H	mg/dl	Optimal: < 100 Near/Above Optimal: 100 - 129 Borderline High: 130 - 159 High: 160 - 189 Very High: > 190	Homogeneous enzymatic colorimetric assay
VLDL CHOLESTEROL	16		mg/dL	< 30	Calculation
NON-HDL CHOLESTEROL	158	H	mg/dL	< 140	Calculation
TRIGLYCERIDES	80		mg/dl	Normal: < 150 Borderline High: 150 - 199 High: 200 - 499 Very High: > 500	Enzymatic colorimetric assay
TOTAL CHOLESTEROL / HDL RATIO	3.5	--	--	< 4.5	Calculation
LDL / HDL RATIO	2.2	--	--	< 3.5	Calculation

Sample Type : Serum

End of Report

Dr. Adley Mark Fernandes
M.D (Pathology)
Pathologist

Dr. Vyoma V Shah
M.D (Pathology)
Clinical Pathologist

This is an electronically authenticated report

Page 2 of 4



BHAVYA THENDANKANDY
Biochemistry Technologist

Printed on: 11/10/2023 16:13

Test result pertains only to the sample tested and to be interpreted in the light of clinical history. These tests are accredited under ISO 15189:2012 unless specified by (^). Test marked with # is performed in an accredited referral laboratory.



Laboratory Investigation Report



BML282607

Name : Ms. JOHARI DONDAPATI
DOB : 26/04/1973
Age / Gender : 50 Y / Female
Referred by : DR RASHMI
Centre : Peshawar Medical Center LLC

Ref No. : 41133
Sample No. : 2310286160
Collected : 11/10/2023 11:00
Registered : 11/10/2023 13:38
Reported : 11/10/2023 15:04

HEMATOLOGY

Test	Result	Flag	Unit	Reference Range	Methodology
COMPLETE BLOOD COUNT (CBC)					
HEMOGLOBIN	12.6		g/dL	12 - 15.5	Spectrophotometry (Oxyhemoglobin)
RBC COUNT	4.6		10 ⁶ /μL	3.9 - 5	Electrical Impedance
HEMATOCRIT	37.6		%	35 - 45	Calculation
MCV	81.4	L	fL	82 - 98	Calculation
MCH	27.3		pg	27 - 32	Calculation
MCHC	33.6		g/dL	32 - 37	Calculation
RDW	13.1		%	11.9 - 15.5	Calculation
RDW-SD	38.1		fL		Calculation
MPV	9.3		fL	7.6 - 10.8	Calculation
PLATELET COUNT	271		10 ³ /μL	150 - 450	Electrical Impedance
PCT	0.3		%	0.01 - 9.99	Calculation
PDW	16.2		Not Applicable	0.1 - 99.9	Calculation
NUCLEATED RBC (NRBC) [^]	0.1		/100 WBC		Flow Cytometry
ABSOLUTE NRBC COUNT [^]	0.01		10 ³ /uL		Calculation
EARLY GRANULOCYTE COUNT (EGC) [^]	0.3		%		Flow Cytometry
ABSOLUTE EGC [^]	0		10 ³ /uL		Calculation
WBC COUNT	8.9		10 ³ /μL	4 - 11	Electrical Impedance
DIFFERENTIAL COUNT (DC)					
NEUTROPHILS	52		%	40 - 75	Flow Cytometry
LYMPHOCYTES	40		%	30 - 60	Flow Cytometry
EOSINOPHILS	2		%	0 - 6	Flow Cytometry
MONOCYTES	5		%	1 - 6	Flow Cytometry
BASOPHILS	1		%	0 - 1	Flow Cytometry
ABSOLUTE COUNT					
ABSOLUTE NEUTROPHIL COUNT	4.7		10 ³ /uL	1.6 - 8.25	Calculation
ABSOLUTE LYMPHOCYTE COUNT	3.6		10 ³ /uL	1.2 - 6.6	Calculation
ABSOLUTE MONOCYTE COUNT	0.4		10 ³ /uL	0.04 - 0.66	Calculation
ABSOLUTE EOSINOPHIL COUNT	0.1		10 ³ /uL	0 - 0.66	Calculation
ABSOLUTE BASOPHIL COUNT	0.1		10 ³ /uL	0 - 0.11	Calculation

Dr. Adley Mark Fernandes
M.D (Pathology)
Pathologist

Dr. Vyoma V Shah
M.D (Pathology)
Clinical Pathologist

This is an electronically authenticated report

Page 3 of 4

Christeena


CHRISTEENA FRANCIS
Laboratory Technologist

Printed on: 11/10/2023 16:13

Test result pertains only to the sample tested and to be interpreted in the light of clinical history. These tests are accredited under ISO 15189:2012 unless specified by (^). Test marked with # is performed in an accredited referral laboratory.



Laboratory Investigation Report



BML282607

Name : Ms. JOHARI DONDAPATI
DOB : 26/04/1973
Age / Gender : 50 Y / Female
Referred by : DR RASHMI
Centre : Peshawar Medical Center LLC

Ref No. : 41133
Sample No. : 2310286160
Collected : 11/10/2023 11:00
Registered : 11/10/2023 13:38
Reported : 11/10/2023 15:04

HEMATOLOGY


Test	Result	Flag	Unit	Reference Range	Methodology
------	--------	------	------	-----------------	-------------

COMPLETE BLOOD COUNT (CBC)

Interpretation Notes : Please note update on CBC report format and changes in reference ranges.

Sample Type : EDTA Whole Blood

End of Report

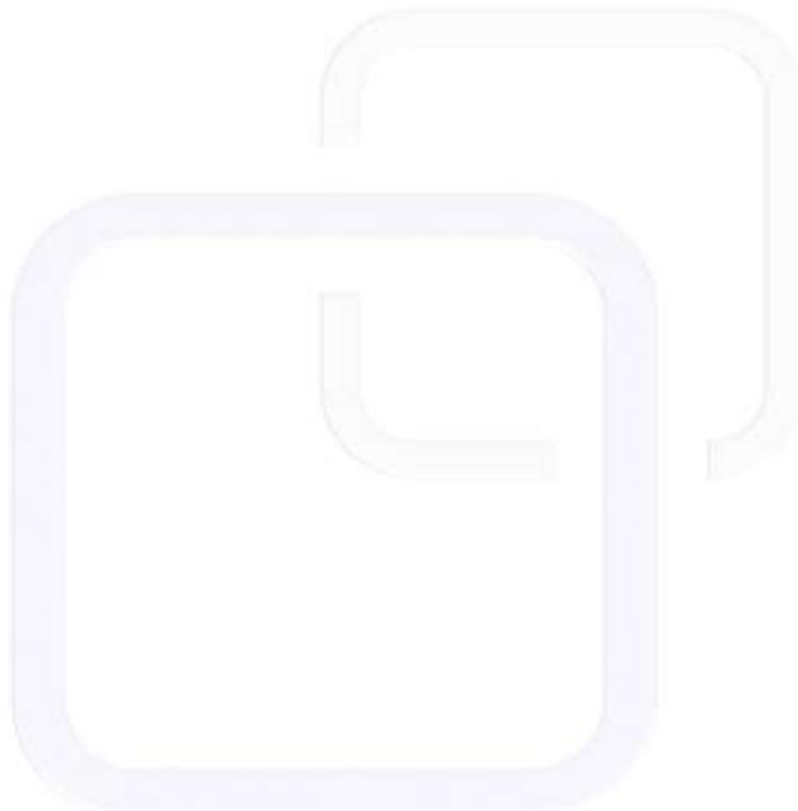

Dr. Adley Mark Fernandes
M.D (Pathology)
Pathologist

Dr. Vyoma V Shah
M.D (Pathology)
Clinical Pathologist

This is an electronically authenticated report

Page 4 of 4

Christeena

CHRISTEENA FRANCIS
Laboratory Technologist

Printed on: 11/10/2023 16:13

Test result pertains only to the sample tested and to be interpreted in the light of clinical history. These tests are accredited under ISO 15189:2012 unless specified by (^). Test marked with # is performed in an accredited referral laboratory.

