



Laboratory Investigation Report

Name : GIUSEPPE MANZELLA
DOB : 24/03/1989
Age / Gender : 35 Y / Male
Referred by : Dr. Enomen Goodluck Ekata
Centre : CITICARE MEDICAL CENTER

Ref No. : 44245
Sample No. : 2409482438
Collected : 30/09/2024 10:50:00
Registered : 30/09/2024 16:41:34
Reported : 02/10/2024 19:19:08

MICROBIOLOGY

Test : CULTURE AND SENSITIVITY (THROAT SWAB)
Specimen : Throat Swab

ResultType : No Bacterial Pathogen Detected after 48 Hours of Aerobic Incubation.

End of Report

Dr. Adley Mark Fernandes
M.D (Pathology)
Pathologist

Dr. Vyoma V Shah
M.D (Pathology)
Clinical Pathologist

This is an electronically authenticated report
Final Report


FATHIMA MUHAMMED SAFIR

Microbiology Technologist
Printed on: 02/10/2024 19:21

Page 1 of 1

Test result pertains only to the sample tested and to be interpreted in the light of clinical history. These tests are accredited under ISO 15189:2012 unless specified by (^). Test marked with # is performed in an accredited referral laboratory.





BML471988

Laboratory Investigation Report

Name : Mr. GIUSEPPE MANZELLA
DOB : 24/03/1989
Age / Gender : 35 Y / Male
Referred by : Dr. Enomen Goodluck Ekata
Centre : CITICARE MEDICAL CENTER


Ref No. : 44245
Sample No. : 2409482438
Collected : 30/09/2024 10:50
Registered : 30/09/2024 16:41
Reported : 30/09/2024 17:27

IMMUNOLOGY

Test	Result	Flag	Unit	Reference Range	Methodology
RAPID INFLUENZA TEST					
Rapid Influenza A	Negative			Negative	Immunochromatography
Rapid Influenza B	Negative			Negative	Immunochromatography

Sample Type : Throat / Nasal swab

End of Report

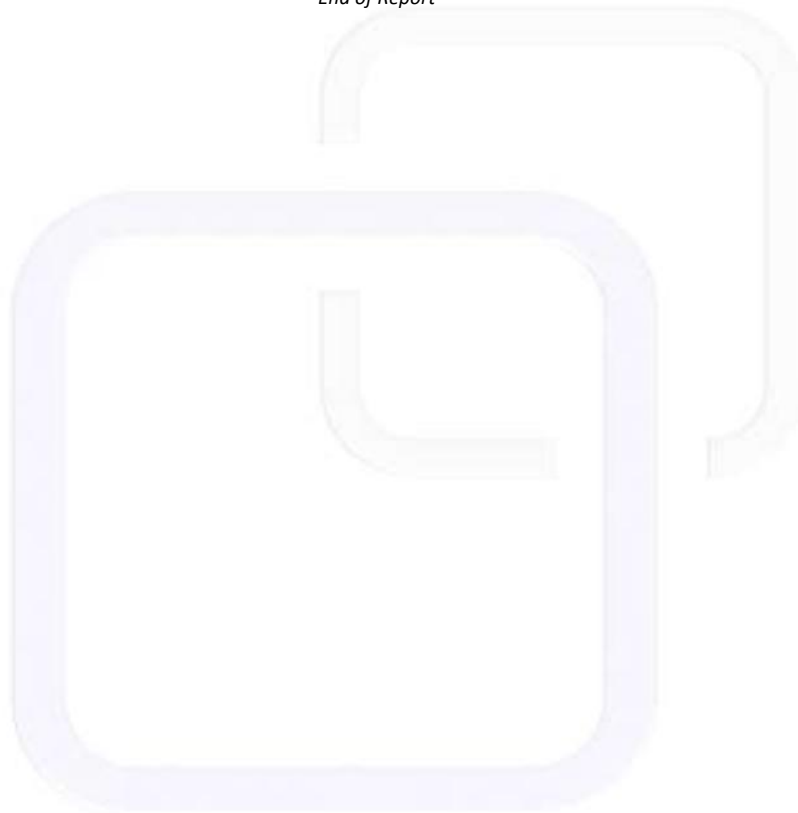

Dr. Adley Mark Fernandes
M.D (Pathology)
Pathologist

This is an electronically authenticated report

Vyoma V. Shah
Dr. Vyoma V Shah
M.D (Pathology)
Clinical Pathologist

Page 1 of 1

Mubasher
MUBASHER ZAHOOR
Laboratory Technologist

Printed on: 02/10/2024 19:21

Test result pertains only to the sample tested and to be interpreted in the light of clinical history. These tests are accredited under ISO 15189:2012 unless specified by (^). Test marked with # is performed in an accredited referral laboratory.

